





INFANT HIP EXAM TRAINER

42000

42010

42004

42014

FOR MORE SKILLS TRAINING PRODUCTS VISIT

limbsandthings.com

INDEX

PACKAGE SUPPLIED	2
SET UP	3
GETTING THE INFANT HIP EXAM TRAINER READY	
CHANGING MODULES	
SAFETY & CLEANING INSTRUCTIONS	4

PACKAGE SUPPLIED


Infant Hip Exam - Upper

42001

42011




Illustration Card



Infant Hip Exam - Lower Normal

42002


42012

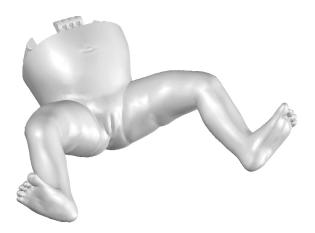


Infant Hip Exam - Lower Abnormal

42003

42013

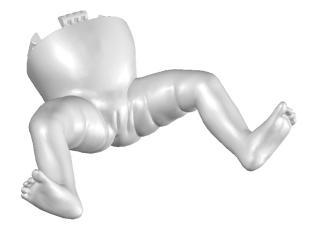

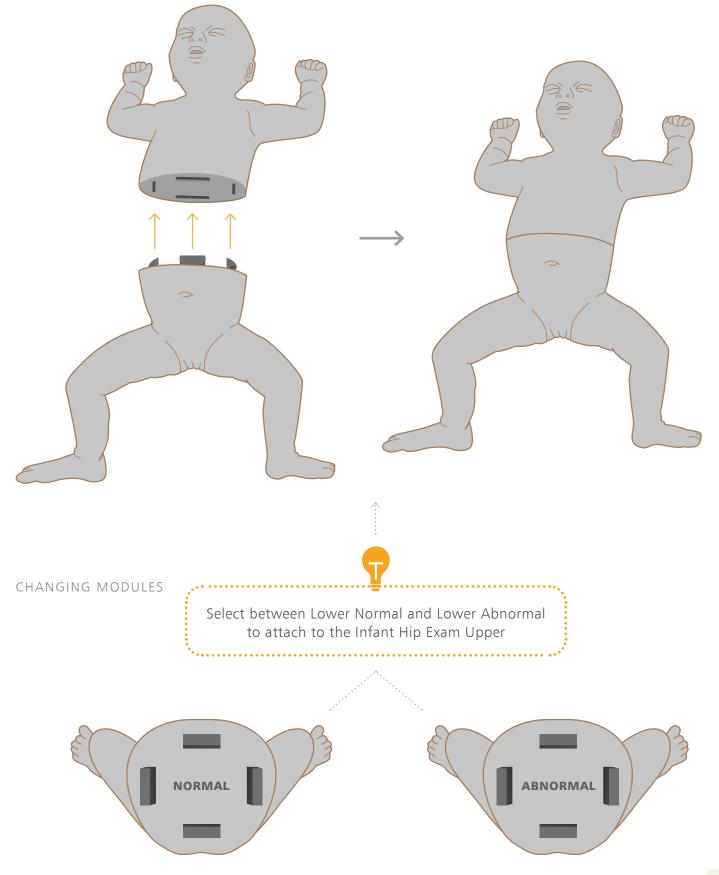

DO's



Follow all instructions. Keep these instructions. Heed all warnings.

Only use attachments/accessories specified by Limbs & Things.





Refer all servicing to qualified service personnel. Servicing is required when the apparatus has been damaged.

Wear gloves at all times and remove all jewellery items. Sharp surfaces such as finger nails and rings can lead to damage of silicone parts.



Clean with a damp soft cloth or sponge, using only warm water with mild detergent.



DON'Ts

Do not abduct the leg by more than 90 degrees





Do not install near any heat sources, do not expose the product to flames or use near naked flame sources. Do not use flammable solvents near or on this product.

Do not set up the product near electrical appliances or items damaged by water.





Do not disassemble the product or attempt to repair a faulty unit, please return the product to Limbs & Things for assessment and repair.

STORAGE & TRANSPORTATION



Always ensure that the product is properly packed and secured during transportation and storage in order to prevent personal injury or damage to the product.

TAKE A LOOK AT Our **video**

VISIT THE WEBSITE limbsandthings.com

OR YOUTUBE CHANNEL youtube.com/limbsandthings





SCAN ME



Part No: 265-503

Issue 04, October 2024 © 2024 Limbs & Things